

# Perfect Prime

## Air quality detector Instruction of AQ9600



[www.perfect-prime.com](http://www.perfect-prime.com)

[cs@perfect-prime.com](mailto:cs@perfect-prime.com)

Please register product warranty on our website

## **Table of Content**

**I. Product overview**

**II. Considerations**

**III. Product description**

**IV. Function setting operation**

**V. Measurement**

**VI. New air quality level**

**VII. Charging**

**VIII. Product specification**

## I. Product overview


AQ9600 has the function of measuring PM2.5, PM10, counting of dust particles, temperature and humidity. The product is provided with high measurement precision, stable performance and simple operation and convenient to carry. It is suitable for indoor environment of family, office, inside of cars and natural environment, etc.

## II. Considerations

1. The electronic sensors and microprocessors used on the product belong to precision electronic device. The product must be kept away from water, fire, inflammable oil and gas or sites with strong electromagnetic interference to prevent influence on/damage to the device.
2. Don't block; or avoid strong air or hot air blowing to the air inlet for air sampling.
3. Please use dry cloth to wipe the instrument case. Don't use damp cloth or corrosive detergents.
4. Don't dismantle and remodel the product without authorization.

## III. Product description

### 1. Product structure and appearance description

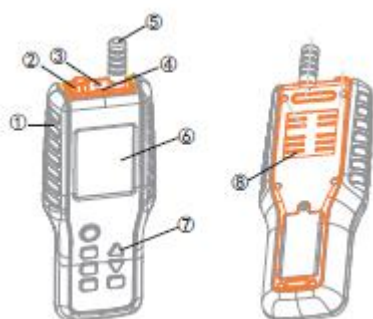


1	Case
2	Temperature and humidity detection port
3	9V/500mA power supply and charging interface
4	USB power supply interface
5	Sampling air inlet
6	LCD display screen
7	Keys
8	Exhaust port

## 2. LCD display description

Number	Display description
1	Hour/minute/second
2	Year/month/day
3	Battery level indication
4	Counting unit
5	Schematic diagram of concentration grade
6	Display area of particle counting
7	Humidity
8	Temperature
9	Measuring object
10	Weight unit
11	Display area of particle weight calculation



## 3. Key function description



Key number	Key name and brief function
1	Power key [⏻]: press to power on/off.
2	Operating measurement key [RUN] (1) At the main interface, press to start data sampling. (2) During the sampling period of 50s, other keys are disabled and cannot operate. Only power key can function.
3	Enter key [ENTER] (1) At the mode of historical record, press--confirm the page number of the selected pages. (2) At the mode of functional parameters, press—confirm to enter function change. (3) At the mode of functional parameters, press—confirm the saved items after change.
4	SHIFT key [SHIFT] (1) At the mode of historical record, press—select the unit's place, ten's place and hundred's place of page number. (2) At the mode of functional parameters, press—select the functional parameter items to be changed.
5	Page up key [▲] (1) At the mode of historical record, used to increase by 1 (+1) and page up by one page. (2) At the mode of functional parameters and at the change state: used to increase by 1 (+1); switching unit and select “yes” or “No”.
6	Page down key [▼] (1) At the main interface, press in order to enter the historical record→the functional parameter. (2) At the mode of historical record, used to decrease by 1 (-1) and page down by one page. At the mode of functional parameters and at the change state: used to decrease by 1 (-1); switching unit and select “yes” or “No”.
7	Back key [BACK] (1) At the mode of historical record and functional parameters, press—back to the main interface. (2) At the mode of historical record, when to change a parameter, press—exit from the change.

#### IV. Function setting operation







Function type	Function items	Function setting operation
Historical record	Page number: Unit's place/ten's place/hundred's place	Check historical record: at the main interface, press [▼] key to enter historical record mode; press [ENTER] key and the current page is selected. At the moment, press [▲] key or [▼] key to go through the data. If you want to skip to certain page directly, input the page number directly. Press [SHIFT] key to select the unit's place, ten's place and hundred's place of the page number. Press [▲] key to increase the value by 1 (+1) and press [▼] key to decrease the value by 1 (-1).
Functional parameters	Particle unit: piece/L, ug/m <sup>3</sup>	Change the particle unit: at the main interface, press [▼] key twice to enter the functional parameter mode, press [ENTER] key to enter the change state. Press [SHIFT] key to select piece/L or ug/m <sup>3</sup> . At the moment, press [▲] key or [▼] key to select your desirable unit and press [ENTER] key to confirm. Press [BACK] key to return to the main interface.
	Time change	At the main interface, press [▼] key twice to enter the functional parameter mode, press [ENTER] key to enter the change state. Press [SHIFT] three times to select "No" in the item of "changing time". Press [▲] key or [▼] key to select "Yes". Press [ENTER] key to enter time change interface. Press [SHIFT] key to select the items to be changed. Press [▲] key to increase the value by 1 (+1) and press [▼] key to decrease the value by 1 (-1). Press [ENTER] to confirm. Press [BACK] key to return to the main interface.
	Temperature unit: °C/°F	At the main interface, press [▼] key twice to enter the functional parameter mode, and press [ENTER] key to enter the change state. Press [SHIFT] key six times to select the items to be changed in "temperature unit". Press [▲] key or [▼] key to select "degree centigrade" or "Fahrenheit degree". Press [ENTER] key to confirm. Press [BACK] key to return to the main interface.
	Restore factory-set value	At the main interface, press [▼] key twice to enter the functional parameter mode, and press [ENTER] key to enter the change state. Press [SHIFT] key seven times to select the items to be changed in "Restore factory-set value". Press [▲] key or [▼] key to select "Yes". Press [ENTER] key to confirm. The screen displays "restoring factory set value...". After completion, press [BACK] key to return to the main interface. (Users may also use the method to delete data record).

## V. Measurement




The instrument should be placed in an open space before measurement to avoid blocking of the sensors. Press the power key to switch on. Press [RUN] key at the main interface and the instrument will enter the sampling state of 50 seconds. At the moment, do not operate the instrument first. After completion of sampling, the measurement result will be displayed on the display screen finally. Users may enter "functional parameter" interface to set the particle unit so as to realize the switching of measurement mode (counting mode/weighing mode).

Note: don't carry out measurement at the time of charging in order to achieve a more accurate measurement result.

## VI. New air quality standard

Schematic diagram of concentration grade	Air quality level	PM2.5 average standard value in 24 hours.
	Excellent	0-35
	Good	35-75
	Slight pollution	75-115
	Moderate pollution	115-150
	Heavy pollution	150-250
	Serious pollution	>250

## VII. Charging

1. The device is provided with the function of display of battery level. When the battery level symbol is displayed as  or , please charge in time.
2. When the adapter is inserted to charge the device, this should be done after powering off. It takes 2 to 3 hours to charge from empty battery to a full battery. When it is fully charged, the battery symbol is . The charging should be stopped at the moment.
3. Charging should be made in a cool and ventilated room. If the surrounding temperature is too high, this may cause abnormal heat of the battery and circuit board or even explosion.
4. Charging may also be made by connecting with a computer through USB. But such method is not good for the instrument's service life and suggested to be used seldom.

## VIII. Product specification

Principle of PM2.5 Sensors	Optoelectronic type
Sampling method	Pumping type
Light sources	Laser diode
Grain size channels	0.3um 2.5um 10 um
Flowrate	1L/min
Measurement range	0-1000ug/m <sup>3</sup>
Resolution ratio	1 ug
Test method	Manual
Sampling time	50s
Sampling method	Pumping type
Typical precision	<20%
Concentration unit	Piece/L   ug/m <sup>3</sup>
Temperature range	0 ~ 50°C
Typical precision	± 1°C
Humidity range	0 ~ 99%RH
Typical precision	±2%RH
Work temperature	-10~50°C
Working humidity	10 ~ 90%RH
Stored data	999 sets
Automatic power off	2 minutes(no key operation)
Technical specification of adapter	Input: AC100~240V -50/60Hz; output: 9VDC, 500mA
Power supply	7.4V chargeable lithium battery
USB	May provide power (unable to download data)
Startup current	120mA
Working current	200mA
Display method	LCD value display. Color backlight
Screen size	2.8 inches
Screen resolution	320*240
Reset	325g (battery included)
Dimension	245 × 85 × 40mm